

**KAMIYA BIOMEDICAL COMPANY**

# **Total Glutathione Quantification Kit**

**For the quantification of total glutathione**

**Cat. No. KT-767**

**For Research Use Only.**

**PRODUCT INFORMATION****Total Glutathione Quantification Kit  
Cat. No. KT-767****PRODUCT**

Glutathione (GSH) is the most abundant thio l(SH) compound in animal tissues, plant tissues, bacteria and yeast. GSH plays many different roles such as protection against reactive oxygen species and maintenance of protein SH groups. During these reactions, GSH is converted into glutathione disulfide (GSSG: oxidized form of GSH). Since GSSG is enzymatically reduced by glutathione reductase, GSH is the dominant form in organisms.

DTNB (5,5'-Dithiobis(2-nitrobenzoic acid)) and glutathione (GSH) react to generate 5-mercapto-2-nitrobenzoic acid and glutathione disulfide (GSSG). Since 5-mercapto-2-nitrobenzoic acid is a yellow colored product, GSH concentration in a sample solution can be determined by the measurement at 412 nm absorbance. GSH is generated from GSSG by glutathione reductase, and reacts with DTNB again to produce 5-mercapto-2-nitrobenzoic acid. Therefore, this recycling reaction improves the sensitivity of total glutathione detection (Fig. 1).

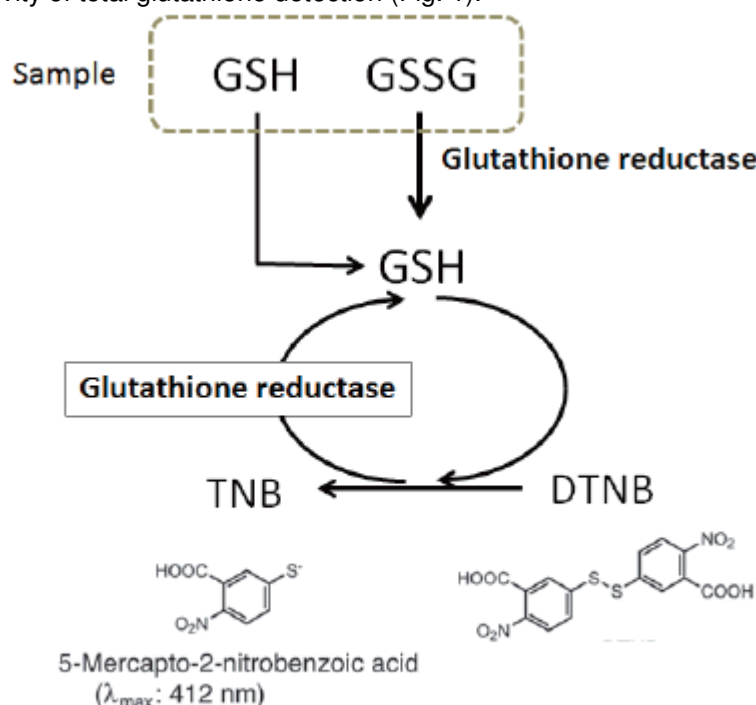


Fig. 1. Principle of Total Glutathione Quantification Kit

**COMPONENTS**

- Substrate (DTNB) x 2
- Coenzyme x 2
- Buffer solution 50 mL x 1
- Enzyme solution 50 μL x 1
- GSH Calibrator x 1

**Materials or equipment required but not provided**

- Microplate reader (with 405 nm filter or 415 nm filter)
- 20 μL, 200 μL and multi-channel pipettes
- 5-Sulfosalicylic acid (SSA)
- 96-well microplate
- Incubator (37°C)

## PROCEDURE

### Precautions

1. Use the reagents in the kit after the reagents temperatures are equilibrated to the room temperature.
2. Triplicate measurements per sample is recommended to obtain accurate data.
3. Since the colorimetric reaction starts immediately after the addition of Substrate working solution to a well, use a multi-channel pipette to avoid the reaction time lag of each well.
4. If the concentration range of total glutathione in a sample is not known, prepare multiple-diluted sample solutions.
5. This kit contains glass vials with an aluminium cap. Please handle carefully.

### Preparation of Solutions

#### Substrate working solution

Add 1.2 mL of Buffer solution to one vial of Substrate, and dissolve.

\*Store the remaining solution at  $-20^{\circ}\text{C}$  (stable at  $-20^{\circ}\text{C}$  for 2 months).

#### Enzyme working solution

Mix Enzyme solution using pipette. Take out 20  $\mu\text{L}$  of Enzyme solution, and mix it with 4 mL of Buffer solution.

\*Store the remaining solution at  $4^{\circ}\text{C}$  (stable at  $4^{\circ}\text{C}$  for 2 months).

#### Coenzyme working solution

Add 1.2 mL of ddH<sub>2</sub>O to the Coenzyme vial, and dissolve.

\*The Coenzyme vial is decompressed; carefully open the cap or use a syringe to add ddH<sub>2</sub>O.

\*Store the remaining solution at  $-20^{\circ}\text{C}$  (stable at  $-20^{\circ}\text{C}$  for 2 months).

#### GSH calibrator solutions

1) Add 2 mL of 0.5% SSA to the Calibrator GSH vial, and dissolve to prepare 200  $\mu\text{mol/L}$  GSH calibrator solution.

\*The Calibrator GSH vial is decompressed; carefully open the cap or use a syringe to add SSA.

\*Store the remaining solution at  $-20^{\circ}\text{C}$  (stable at  $-20^{\circ}\text{C}$  for 2 months).

2) Dilute 100  $\mu\text{L}$  of 200  $\mu\text{mol/L}$  GSH calibrator solution by serial dilution with 100  $\mu\text{L}$  of 0.5% SSA in plastic tubes as indicated in Fig. 2.

\*GSH calibrator solutions: 100  $\mu\text{mol/L}$ , 50  $\mu\text{mol/L}$ , 25  $\mu\text{mol/L}$ , 12.5  $\mu\text{mol/L}$ , 6.25  $\mu\text{mol/L}$ , 3.13  $\mu\text{mol/L}$ , 1.56  $\mu\text{mol/L}$  and 0  $\mu\text{mol/L}$ .

\*Use up the solution within one day.

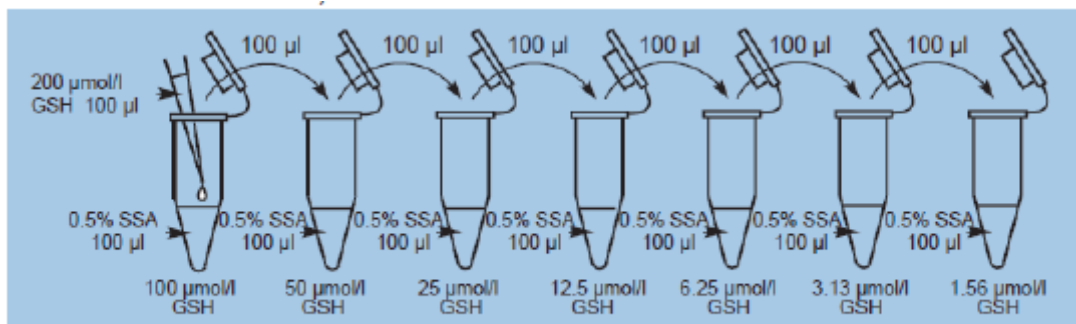


Fig. 2 Preparation of GSH standard solutions.

### Total glutathione detection

#### Detection range: 5-100 $\mu\text{mol/L}$

- 1) To each well, add 20  $\mu\text{L}$  of Coenzyme working solution, 120  $\mu\text{L}$  of Buffer solution and 20  $\mu\text{L}$  of Enzyme working solution.
  - 2) Incubate the plate at  $37^{\circ}\text{C}$  for 5 minutes.
  - 3) Add 20  $\mu\text{L}$  of either one of the GSH calibrator solutions or the sample solutions.
- \*Adjust the concentration of SSA in the sample solution to 0.5-1% with ddH<sub>2</sub>O before the assay. High concentrations of SSA ( $>1\%$ ) interfere with the assay. See Fig. 3 for a plate diagram of the solution arrangement.
- 4) Incubate the plate at  $37^{\circ}\text{C}$  for 10 minutes.
  - 5) Add 20  $\mu\text{L}$  of Substrate working solution, and incubate the plate at room temperature for 10 minutes.
  - 6) Read the absorbance at 405 nm or 415 nm using a microplate reader.
  - 7) Determine concentrations of GSH in the sample solutions using a calibration curve.
- \*Since the colorimetric reaction is stable and the O.D. increases linearly over 30 minutes, GSH concentration can be determined by using kinetic or pseudo-end point (no stopping reaction, quick measurement of the O.D. at certain

time points between 5 and 10 minutes) methods.

\*Typical calibration curves prepared using the kinetic method and the pseudo-end point method are indicated in Fig. 4 and 5, respectively.

### Detection range: 0.5-25 $\mu\text{mol/L}$

Change the procedure as follows:

- Prepare GSH calibrator solutions by serial dilution with 0.5% SSA as follows:  
25  $\mu\text{mol/L}$ , 12.5  $\mu\text{mol/L}$ , 6.25  $\mu\text{mol/L}$ , 3.13  $\mu\text{mol/L}$ , 1.56  $\mu\text{mol/L}$ , 0.78  $\mu\text{mol/L}$ , 0.39  $\mu\text{mol/L}$  and 0  $\mu\text{mol/L}$ .
- Incubate the plate at room temperature for 20-40 min after adding Substrate working solution.

	1	2	3	4	5	6	7	8	9	10	11	12
A	Blank											
B	1.56 $\mu\text{mol/L}$ GSH											
C	3.13 $\mu\text{mol/L}$ GSH											
D	6.25 $\mu\text{mol/L}$ GSH						Sample					
E	12.5 $\mu\text{mol/L}$ GSH											
F	25 $\mu\text{mol/L}$ GSH											
G	50 $\mu\text{mol/L}$ GSH											
H	100 $\mu\text{mol/L}$ GSH											

Fig. 3 Plate Diagram: an example of the GSH standard solution and sample solution arrangement to be measured in triplicate (up to 24 samples can be determined in one plate).

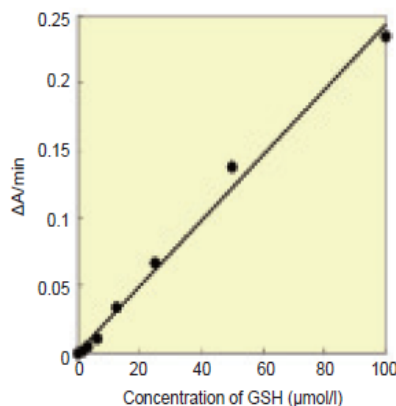


Fig. 4 Calibration curve prepared using kinetic method.

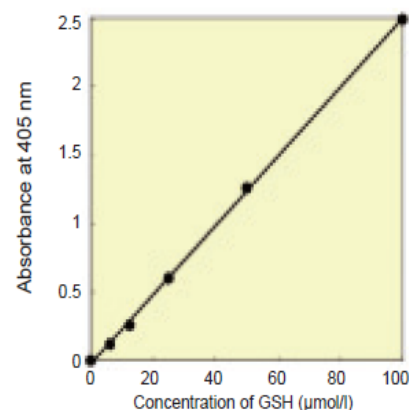


Fig. 5 Calibration curve prepared using pseudo-end point method.

### Calculation of total glutathione (GSH and GSSG) concentration

Determine the total glutathione concentration a) in a sample solution using the following equations.

Pseudo-end point method:

$$\text{Total glutathione} = (\text{O.D.sample} - \text{O.D.blank}) / \text{slope}$$

Kinetic method:

$$\text{Total glutathione} = (\text{Slope}^c \text{ sample} - \text{Slope}^c \text{ blank}) / \text{slope}^b$$

a) Since the values obtained by these equations are the amount of total glutathione in treated sample solutions, further calculations are necessary if the actual concentrations of glutathione in cells or tissues need to be determined.

b) slope of the calibration curve.

c) slope of the kinetic reaction.

### INTERFERENCE

Reducing agents such as ascorbic acid,  $\beta$ -mercaptoethanol, dithiothreitol (DTT) and cysteine, or thiol reactive compounds such as maleimide compounds, interfere with the glutathione assay. Therefore, SH compounds, reducing agents and SH reactive materials should be avoided during the sample preparation.

### STORAGE

Store the kit at 4°C. Substrate working solution, Coenzyme working solution and GSH calibrator solution can be stored at -20°C for 2 months. Enzyme working solution is stable for 2 months at 4°C (Do not freeze).

## FOR RESEARCH USE ONLY

### KAMIYA BIOMEDICAL COMPANY

12779 Gateway Drive, Seattle WA 98168

Tel: (206) 575-8068 Fax: (206) 575-8094

Email: LifeScience@k-assay.com

www.k-assay.com